



LJMU Research Online

Bogerd, CP, Velt, KB, Annaheim, S, Bongers, CCWG, Eijsvogels, TMH and Daanen, HAM

Comparison of two telemetric intestinal temperature devices with rectal temperature during exercise.

<http://researchonline.ljmu.ac.uk/id/eprint/8092/>

Article

Citation (please note it is advisable to refer to the publisher's version if you intend to cite from this work)

Bogerd, CP, Velt, KB, Annaheim, S, Bongers, CCWG, Eijsvogels, TMH and Daanen, HAM (2018) Comparison of two telemetric intestinal temperature devices with rectal temperature during exercise. Physiological Measurement. ISSN 0967-3334

LJMU has developed [LJMU Research Online](#) for users to access the research output of the University more effectively. Copyright © and Moral Rights for the papers on this site are retained by the individual authors and/or other copyright owners. Users may download and/or print one copy of any article(s) in LJMU Research Online to facilitate their private study or for non-commercial research. You may not engage in further distribution of the material or use it for any profit-making activities or any commercial gain.

The version presented here may differ from the published version or from the version of the record. Please see the repository URL above for details on accessing the published version and note that access may require a subscription.

For more information please contact researchonline@ljmu.ac.uk

<http://researchonline.ljmu.ac.uk/>

1 Title: Comparison of two telemetric intestinal temperature devices with rectal temperature during
2 exercise

3

4 Authors: CP Bogerd¹, KB Velt^{1,2}, S Annaheim³, CCWG Bongers⁴, TMH Eijsvogels^{4,5}, HAM Daanen²

5

6 Affiliations:

7 1. TNO, Training and Performance Innovations/CBRN Protection, Postbus 23, 3769 ZG
8 Soesterberg, the Netherlands

9 2. Department of Human Movement Sciences, Faculty of Behavioural and Movement Sciences,
10 Vrije Universiteit Amsterdam, Amsterdam Movement Sciences, De Boelelaan 1105, 1081 HV
11 Amsterdam, The Netherlands

12 3. Empa, Laboratory for Biomimetic Membranes and Textiles, Lerchenfeldstrasse 5, 9014 St.
13 Gallen, Switzerland

14 4. Radboud Institute for Health Sciences, Radboud university medical center, Department of
15 Physiology, P.O. Box 9101, 6500 HB Nijmegen, The Netherlands

16 5. Research Institute for Sports and Exercise Sciences, Liverpool John Moores University, Byrom
17 Street, Liverpool L3 3AF, United Kingdom

18 **Summary**

19 The experienced discomfort of rectal probes and esophageal probes for the estimation of body core
20 temperatures has triggered the development of GI-capsules that are easy acceptable for athletes and
21 workers due to their non-invasive characteristics.

22 We compare two new GI-capsule devices with rectal temperature during cycle ergometer exercise and
23 rest. Eight participants followed a protocol of (i) 30 min exercise with a power output of 130 W, (ii)
24 5 min rest, (iii) 10 min self-paced maximum exercise, and (iv) 15 min rest. Core temperature was
25 measured using two GI-capsule devices (e-Celsius and myTemp) and rectal temperature.

26 The myTemp system gave temperatures indifferent different from rectal temperature during rest and
27 exercise. However, the factory calibrated e-Celsius system, showed a systematic underestimation of
28 rectal temperature of 0.2 °C that is corrected in the 2018 versions. Finally, both GI-capsules react
29 faster to temperature changes in the body compared to the rectal temperature probe during the rest
30 period following maximum exercise.

31

32 Keywords: core temperature, gastrointestinal temperature, comparison, telemetric temperature
33 measurement, myTemp, e-Celsius

1 Introduction

2 It is well established that endurance performance is compromised with uncompensable heat-stress
3 (Cheung *et al.* 2000) where high body core temperatures are attained (Gonzalez-Alonso *et al* 1999).
4 Furthermore, heat tolerance and thus high core temperatures is dependent on training status (Cheung
5 and McLellan 1998). Therefore, athletes use both internal cooling, e.g., with an ice slurry (Siegel *et al*
6 2010) or external cooling such as cooling vests or ice pads (Bogerd *et al* 2010, Bongers *et al* 2017a)
7 prior to or during exercise to reduce heat strain, i.e., to keep the core temperature lower compared
8 to the absence of a cooling intervention. The thermal balance during exercise is not easy to maintain
9 since high levels of metabolic heat production, often exceeding 1000 W, have to be exactly matched
10 by heat loss. A discrepancy between metabolic heat production and heat loss will lead to hypothermia
11 or hyperthermia. Severe cases of hyperthermia has been reported at the end of a marathon among
12 finishing athletes (Roberts 2007). Hypothermia leads to suboptimal performance, since muscle
13 contractions are less efficient in cool muscles (De Ruiter and De Haan 2001). For hyperthermia it has
14 been shown that gross efficiency drops by about 1% for every 1 °C core temperature increase for core
15 temperatures up to 38.3 °C (Daanen *et al* 2006). In order to maintain optimal performance it is
16 therefore instrumental to monitor exercise-induced changes in core temperature. A few decades ago,
17 gastro-intestinal (GI)-capsules became available that have been validated to be a good estimator of
18 body core temperature (Byrne and Lim 2007, Teunissen *et al* 2012, Mündel *et al* 2016, Towey *et al*
19 2017, Travers *et al* 2016).

20 Although it is well acknowledged that no single core temperature exists and that at each measurement
21 site the local thermal balance defines the temperature (Taylor *et al* 2014), there are some preferred
22 sites for measurement. Rectal temperature is considered to be a good standard for tracking stationary
23 temperatures, but has been shown to have a delayed responsiveness compared to esophageal
24 temperature (Teunissen *et al* 2012). The latter is widely considered as fast and reproducible (Taylor *et*
25 *al* 2014). The advantage of rectal temperature measurements is that the measurement location is
26 reliable and well defined when the probe is inserted at least 7 cm past the anal sphincter (Buono *et al*
27 2014). However, the rectal probe insertion may cause discomfort and typically has a wire connection.
28 Therefore, rectal temperature is not suitable in field based conditions (Ducharme *et al* 2001). GI-
29 capsules are comfortable and easily applicable in both lab and field conditions, but the location in the
30 body varies and may lead to variations in recorded temperature. Wilkinson *et al.* (2008) reported that
31 cold water ingestion has a strong location specific influence on GI-temperature. To avoid interference
32 between fluid ingestion and core body temperature measurements, it is recommended to abstain
33 from drinking during the experiment, to drink water of 37 °C (Ducharme *et al* 2001) or to ingest the
34 capsule several hours prior the start of the experiment to ensure passage through the stomach (Byrne
35 and Lim 2007), up to about 6 hours (Lee *et al* 2000).

36 This study evaluates two recently developed GI capsule systems (e-Celsius and myTemp) and
37 compares the results with rectal temperature measurements. This is the first in-vivo study evaluating
38 the myTemp GI capsule system with rectal temperature. Previously, we validated the myTemp system
39 ex-vivo (Bongers *et al* 2017b) and compared to e-Celsius and two other systems ex-vivo (Bongers *et al*
40 2018). Differences were found among the systems. However, the validity, test-retest reliability, and
41 inertia were qualified as very well for all systems. These ex-vivo tests were carried out using a water
42 bath, the question remains how these systems perform in-vivo, while participants ingest the capsule
43 and during exercise. Travers *et al* (2016) recently carried out such in-vivo tests compared the e-Celsius

1 system with rectal temperature and with a GI capsule system available on the market since several
2 years (VitalSense). They find that both GI systems underestimate rectal temperature with 0.2 °C. In
3 this study we include the myTemp system and use a different exercise protocol. Travers *et al* (2016)
4 used two different exercise protocols, one mimicking soccer on a treadmill with over 30 changes in
5 running speed during 15 min and a cycle ergometer test with a constant power output. We used an
6 intermittent cycling exercise with fewer changes in power output compared to Travers *et al* (2016),
7 allowing a better insight into the delay between changes in heat production (related to power output)
8 and core temperature measurement site. We hypothesize that the e-Celsius and myTemp system will
9 give comparable results and show less time lag for temperature changes than rectal temperature.

10 **Methods**

11 **Participants**

12 Eight male participants voluntarily participated in this study (age: 32 ± 13 yrs, height: 1.88 ± 0.52 m,
13 weight: 80.0 ± 7.6 kg). Participants were included based on a positive evaluation of a health
14 questionnaire by a physician. The experimental protocol was reviewed and approved by the TNO
15 Ethics Committee in accordance with the Helsinki Declaration of 1975, as revised in 2013. All
16 participants gave written consent prior to inclusion.

17 **Protocol**

18 Participants visited our facilities once. During this visit, participants ingested two GI capsules, one for
19 each GI system, followed by a rest period allowing time for the capsules to pass through the stomach.
20 The time between insertion and onset of measurements was 137 ± 22 minutes. The participants were
21 instructed to wear a T-shirt and shorts. Furthermore, they were not allowed to eat or drink throughout
22 the measurement protocol. Shortly before the start of the measurements the participants inserted a
23 rectal probe (dedicated rectal probe with a DS18B20 temperature sensor, connected with a wire to a
24 logger (MSR, 145WD, Seuzach, Switzerland), additional details are given in Table 2) at least 10 cm
25 beyond the rectal sphincter. The experiment took place in a climatic chamber in order to accurately
26 control the environmental conditions of 29.6 ± 0.1 °C air temperature and $49 \pm 1\%$ humidity (3M,
27 QUESTemp° Heat Stress Monitor QT-44, St. Paul, USA). Upon arrival in the climatic chamber,
28 participants rested for 20 minutes in order to familiarize to the circumstances. Thereafter, the
29 participants performed a 30 minute submaximal exercise with a power output of 130 W on a cycle
30 ergometer (Lode, Lode Excalibur, Groningen, The Netherlands). Hereafter, the participants rested for
31 5 minutes, followed by a maximal exercise phase of 10 minutes on a self-selected pace. All
32 measurements were continued for 15 minutes after exercise cessation. The exercise protocol is
33 summarized in table 1. During the exercise sessions the participants were instructed to keep their
34 cadence constant around a value of their choice, but within 60 – 120 rpm.

35

Table 1. The exercise protocol.

Phase	Duration [min]	Power Output [W]
1 Exercise	30	130
2 Rest	5	0
3 Exercise	10	Self paced maximum
4 Rest	15	0

1

2 Telemetric intestinal temperature devices

3 The characteristics of both capsule systems are presented in table 2; the capsules are similar to
 4 those used to encapsulate medical agents. The e-Celsius system consisted of a GI capsule and a
 5 receiver, referred to as the monitor (BodyCap, Caen, France). Unique to this device is that the
 6 capsule is equipped with a memory chip, which allows storage of data in case of loss of connection
 7 with the monitor. Data stored in the memory is transferred once the connection with the monitor is
 8 restored. The myTemp system (myTemp, Nijmegen, The Netherlands) is a prototype system that is
 9 not yet commercially available. This system consists of a GI capsule and a waist belt. The uniqueness
 10 of the myTemp system is that the capsule lacks a battery. Its energy supply is created through a
 11 magnetic field created by the belt which causes a current in a coil in the capsule. The lifetime of a GI
 12 capsule is usually determined by the battery, but the lifetime of the myTemp capsule is infinite
 13 (according to the manufacturer) due to external energy supply. Absence of a battery will reduce the
 14 environmental pollution. Moreover, the battery is an important cost driver and the MyTemp sensor
 15 system will be less expensive than systems with a battery.

16 The e-Celsius and myTemp systems were factory calibrated. The MSR system for rectal temperature
 17 was calibration in our lab, using a thermostat water bath and an externally calibrated PT-100
 18 temperature sensor including logger (P750, Tservice, Gennep, the Netherlands).

Table 2. Specifications of devices used to measured core temperature.

Brand	Type	Sample Time [s]	Accuracy [°C]	Sensor Location	Capsule Size [mm ²]	Capsule Mass [g]	Capsule storage Datapoints	Capsule data transmission [MHz]	Equiped With Battery	Software name and version
myTemp	*	10	0.01	Intestines	20.0 x 8.0	8.0	0	433	No	e-Performance manager v01.01.00.0C
e-Celsius	Performance	30	0.2	Intestines	17.7 x 8.9	1.7	2000	433	Yes	myTemp Manager v01.08
MSR	145	1	0.1	Rectum	-	-	-	-	-	MSR v5.30.18

*A type name is not yet defined.

19

20 Data processing and statistics


21 Rectal temperature was sampled every second, whereas the myTemp and e-Celsius temperature were
 22 registered every 10 s and 30 s, respectively. The following parameters were derived for each phase of

1 the experimental protocol (i.e., exercise at 130 W, rest, maximum exercise, and second rest): (i) mean
2 core temperature, ii) Root Mean Square Deviation (RMSD) from the capsule systems with rectal
3 temperature as reference (first difference for every data point for each participant between two
4 parameters, then the root of the squared mean), and (iii) maximum core temperature. In order to
5 investigate the differences in response time among the three different devices, the slope in core
6 temperature was obtained from a linear regression analysis on the last 7.5 min of the final rest period.
7 This is the period after the peak temperature. Finally, Bland-Altman plots were used to visualize the
8 deviation for each system from rectal temperature.

9 All data is presented as mean \pm standard deviation, unless indicated otherwise. Statistical analysis was
10 carried out with Statistica 13.1 and IBM SPSS Statistics 24. A two-way repeated measures ANOVA for
11 within participant effect is applied to these parameters to evaluate differences among the three
12 devices used to measure core temperature. A Bonferroni post-hoc test was employed upon statistical
13 significant effects ($p < .05$).

14 Results

15 Figure 1 shows the average core temperatures measured with the three different devices. Table 3
16 gives the results per phase for each device separate for mean temperature, RMSD from the capsule
17 systems with rectal temperature, and maximal temperature. The mean absolute temperatures
18 differed between the three investigated systems ($p = .011$). A post-hoc analysis showed that this is
19 due to consistently lower temperatures for e-Celsius compared to myTemp ($p = .015$). The RMSD
20 indicates that the absolute differences between myTemp and rectal are not different from the
21 absolute differences between e-Celsius and rectal ($p = .268$). There are no differences between the
22 investigated systems for maximum temperature ($p = .058$).

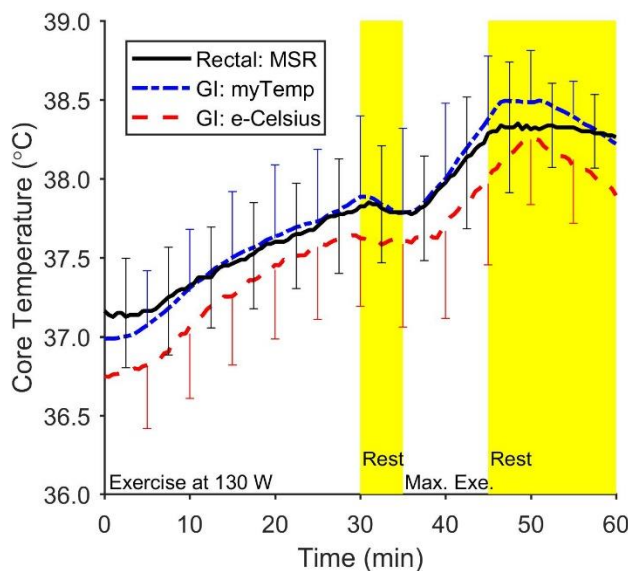

23

24 **Figure 1.** Rectal, myTemp, and e-Celsius temperatures during the four phases as indicated (see also
25 table 1) averaged over all participants. The error-bars indicate \pm one standard deviation for the
26 capsule systems.

27

Table 3. Mean, root mean square deviation, and maximum temperatures for the different devices and phases.

Device	Mean Core Temperature per Phase (°C)				ANOVA*
	Submaximal Exercise	Rest	Maximal Exercise	Rest	
A: Rectal: MSR	37.5 ± 0.3	37.8 ± 0.4	38.0 ± 0.4	38.3 ± 0.3	F = 6.391
B: GI: myTemp	37.4 ± 0.4	37.8 ± 0.5	38.0 ± 0.5	38.4 ± 0.4	p = .011
C: GI: e-Celsius	37.2 ± 0.4	37.6 ± 0.5	37.7 ± 0.5	38.1 ± 0.3	

*Results for the within participant effects, post-hoc analysis revealed: p(a vs. b) = 1.000, p(a vs. c) = .640, p(b vs. c) = .015.

Device	Root Mean Square Deviation of Gastro-Intestinal Core Temperature compared to Rectal Temperature (°C)				ANOVA
	Submaximal Exercise	Rest	Maximal Exercise	Rest	
A: GI: MyTemp	0.19 ± 0.15	0.22 ± 0.18	0.30 ± 0.20	0.24 ± 0.15	F = 1.451
B: GI: e-Celsius	0.30 ± 0.13	0.25 ± 0.15	0.40 ± 0.15	0.31 ± 0.15	P = .268


Device	Maximal Core Temperature per Phase (°C)				ANOVA*
	Submaximal Exercise	Rest	Maximal Exercise	Rest	
A: Rectal: MSR	37.8 ± 0.4	37.9 ± 0.4	38.3 ± 0.4	38.5 ± 0.3	F = 5.516
B: GI: myTemp	37.9 ± 0.4	37.9 ± 0.5	38.4 ± 0.5	38.6 ± 0.4	p = .058
C: GI: e-Celsius	37.7 ± 0.5	37.7 ± 0.5	38.0 ± 0.4	38.3 ± 0.3	

*Results for the within participant effects.

1

2 Bland-Atlman plots are given in figure 2, comparing the three devices to each other. The differences
 3 among the devices show comparable standard deviations ranging between 0.20 °C and 0.27 °C. The e-
 4 Celsius device shows a mean difference (systemic bias) of -0.22 °C and 0.25 °C compared to rectal
 5 temperature and myTemp, respectively. The systemic bias between myTemp and rectal is the closes
 6 to zero with 0.03 °C (figure 2).

7

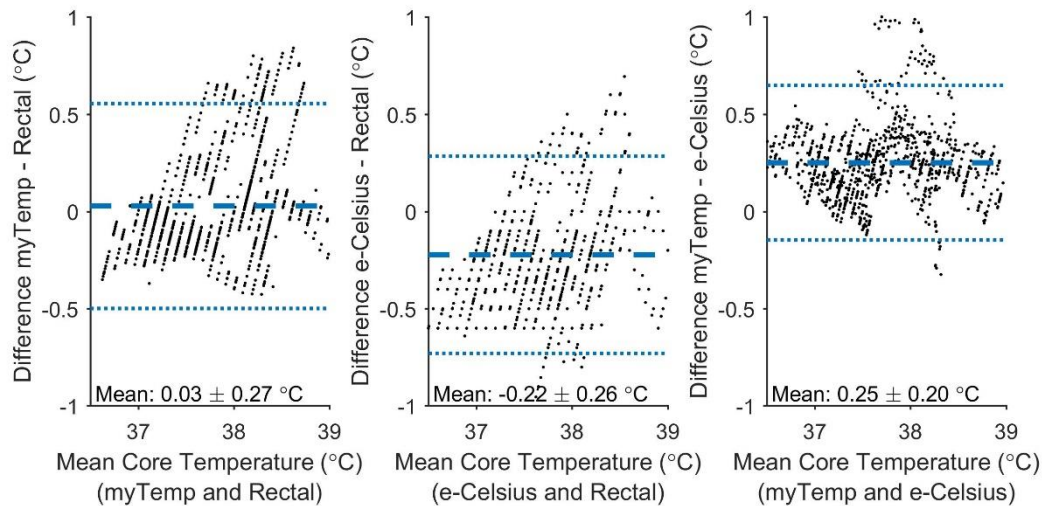

1

2 **Figure 2.** Bland-Altman plots comparing the different devices used for measuring core temperature.
 3 The middle horizontal line (dark blue) indicates the mean difference between two devices, both outer
 4 horizontal lines (light blue) enclose the 95% limits of agreement. The mean difference \pm one standard
 5 deviation are also given per plot.

6 The rate of change in core temperature was obtained from the last 7.5 min of the last rest phase (table
 7 4). This slope indicates the responsiveness of the devices. The slope of rectal temperature was
 8 significantly different from both GI based devices ($F = 11.520$, $p = .001$). Despite interindividual
 9 differences, post-hoc analysis of the one-way ANOVA repeated measures revealed $p = .027$ and
 10 $p = .012$ for myTemp and e-Celsius both compared to rectal, respectively. In fact, the rate of core
 11 temperature decrease was a factor 3.5 and 3.9 faster for myTemp and e-Celsius compared to rectal,
 12 respectively.

Table 4. Rate of change in core temperature ($^{\circ}\text{C}/\text{h}$) during the last 7.5 min per participant as well as mean and standard deviation (std).

Participant	Rectal: MSR	GI: myTemp	GI: e- Celsius
1	0.0	-3.4	-2.9
2	-0.8	-2.0	-3.6
3	-0.3	-2.0	-2.5
4	-1.3	-1.6	-2.1
5	-1.3	-1.0	-1.2
6	1.1	-0.6	0.0
7	0.0	-1.9	-0.9
8	-1.7	-3.0	-4.2
Mean	-0.6	-1.9	-2.2
std	0.9	0.9	1.4

13

1 Discussion

2 The experienced discomfort of rectal probes and esophageal probes for the estimation of body core
3 temperatures has triggered the development of GI-capsules that are easy acceptable for athletes and
4 workers due to their non-invasive characteristics. A recent ex-vivo investigation showed that the
5 myTemp and e-Celsius systems are able to accurately represent fluid temperatures and fast changes
6 in fluid temperatures (Bongers *et al* 2018). The results of the current in-vivo study focusses on the
7 performance of these GI-capsules during exercise and consecutive rest periods.

8 The temperatures of the e-Celsius systems were systematically lower than the rectal values by about
9 0.2 °C averaged over the two exercise and two rest phases. This systematic underestimation of the e-
10 Celsius system was also observed in a recent experiment that compared the e-Celsius system to the
11 Vital Sense system and rectal temperature during running and cycling (Travers *et al* 2016). Both
12 systems showed an underestimation of 0.2 °C compared to the rectal temperature values during
13 cycling and running. This difference was comparable during calibration in water, and led the authors
14 to suggest that calibration of GI-capsules is required prior to their use (Travers *et al* 2016). Our study
15 showed that this does not apply to the myTemp system which can be used without prior calibration.
16 However, the dynamics of the GI system evaluated in this study are very similar as can be observed in
17 figure 2 and table 4.

18 Rectal temperature showed a slower response compared to both the myTemp and e-Celsius systems.
19 This is particularly visible after the maximum exercise phase; the decrease in core temperature after
20 maximal exercise was more than three times faster for the GI-capsules than for rectal temperature.
21 The slow response of rectal temperature is in line with earlier observations (Byrne and Lim 2007, Lee
22 *et al* 2000). If fast changes in body core temperature have to be determined, esophageal temperature
23 seems most appropriate since it closely resembles the temperature of the blood returning from the
24 peripheral tissues (Teunissen *et al* 2012). For steady-state exercise both rectal probes and GI-capsules
25 may be applied of which the latter provide more comfort to the user. A disadvantage of the GI-
26 capsules is that the location of the capsule in the digestive system varies over time and that the
27 temperature profile in the GI-tract is not constant. Every location in the GI-tract can be considered as
28 a local spot with a specific core temperature (Taylor *et al* 2014). Rectal probes, when appropriately
29 inserted, do not have this disadvantage. During exercise and in the absence of drinking fluids,
30 however, the fluctuations in the GI-tract are considered to be small (Towey *et al* 2017).

31 In conclusion, the myTemp system yielded temperatures that were not significantly different from
32 rectal temperature values during rest and exercise. The e-Celsius system, however, showed a
33 systematic bias of 0.2 °C that should be corrected for by calibration prior its use. The GI-capsules react
34 faster to temperature changes in the body compared to the rectal temperature probe in particular in
35 the rest period following exercise.

36 Acknowledgement

37 The authors gratefully acknowledge the e-Celsius and myTemp for providing their system for the
38 purpose of this study.

1 **References**

- 2 Bogerd N, Perret C, Bogerd C, Rossi R M and Daanen H A M 2010 The effect of pre-cooling intensity
3 on cooling efficiency and exercise performance *J. Sports Sci.* **28** 771–9
- 4 Bongers C C W G, Daanen H A M, Bogerd C P, Hopman M T E and Eijsvogels T M H 2018 Validity,
5 Reliability and Inertia of Four Different Temperature Capsule Systems. *Med. Sci. Sports Exerc.*
6 **50** 169-75
- 7 Bongers C C W G, Hopman M T E and Eijsvogels T M H 2017a Cooling interventions for athletes: An
8 overview of effectiveness, physiological mechanisms, and practical considerations *Temperature*
9 **4** 60–78
- 10 Bongers C C W G, Hopman M T E and Eijsvogels T M H 2017b Validity and reliability of the myTemp
11 ingestible temperature capsule *J. Sci. Med. Sport. In press.*
- 12 Buono M J, Holloway B, Levine A, Rasmussen C and Kolkhorst F W 2014 Effect of air temperature on
13 the rectal temperature gradient at rest and during exercise. *Int. J. Physiol. Pathophysiol.*
14 *Pharmacol.* **6** 61–5
- 15 Byrne C and Lim C L 2007 The ingestible telemetric body core temperature sensor: a review of
16 validity and exercise applications *Br. J. Sports Med.* **41** 126–33
- 17 Cheung S S and McLellan T M 1998 Heat acclimation, aerobic fitness, and hydration effects on
18 tolerance during uncompensable heat stress *J. Appl. Physiol.* **84** 1731–9
- 19 Cheung S S, McLellan T M and Tenaglia S 2000 The thermophysiology of uncompensable heat stress.
20 Physiological manipulations and individual characteristics. *Sports Med.* **29** 329–59
- 21 Daanen H A, van Es E M and de Graaf J L 2006 Heat Strain and Gross Efficiency During Endurance
22 Exercise after Lower, Upper, or Whole Body Precooling in the Heat *Int. J. Sports Med.* **27** 379-88
- 23 Ducharme M B, McLellan T M, Moroz D, Buguet A and Radomski M W 2001 A 36-hour comparison of
24 core temperature at rest and during exercise using rectal probe and pill telemetry *Proc. Aust.*
25 *Physiol. Pharmacol. Soc.* **32** 28
- 26 Gonzalez-Alonso J, Teller C, Andersen S L, Jensen F B, Hyldig T and Nielsen B 1999 Influence of body
27 temperature on the development of fatigue during prolonged exercise in the heat *J. Appl.*
28 *Physiol.* **86** 1032–9
- 29 Lee S M, Williams W J and Fortney Schneider S M 2000 Core temperature measurement during
30 supine exercise: esophageal, rectal, and intestinal temperatures. *Aviat. Space. Environ. Med.* **71**
31 939–45
- 32 Mündel T, Carter J M, Wilkinson D M and Jones D A 2016 A comparison of rectal, oesophageal and
33 gastro-intestinal tract temperatures during moderate-intensity cycling in temperate and hot
34 conditions *Clin. Physiol. Funct. Imaging* **36** 11–6
- 35 Roberts W O 2007 Heat and cold: what does the environment do to marathon injury? *Sport. Med.* **37**
36 400–3
- 37 De Ruiter C J and De Haan A 2001 Similar effects of cooling and fatigue on eccentric and concentric
38 force-velocity relationships in human muscle. *J. Appl. Physiol.* **90** 2109–16
- 39 Siegel R, MatÉ J, Brearley M B, Watson G, Nosaka K and Laursen P B 2010 Ice Slurry Ingestion
40 Increases Core Temperature Capacity and Running Time in the Heat *Med. &* **42** 717–25

- 1 Taylor N A S, Tipton M J and Kenny G P 2014 Considerations for the measurement of core, skin and
2 mean body temperatures. *J. Therm. Biol.* **46** 72–101 Online:
- 3 Teunissen L P J, de Haan A, de Koning J J and Daanen H A M 2012 Telemetry pill versus rectal and
4 esophageal temperature during extreme rates of exercise-induced core temperature change.
5 *Physiol. Meas.* **33** 915–24
- 6 Towey C, Easton C, Simpson R and Pedlar C 2017 Conventional and novel body temperature
7 measurement during rest and exercise induced hyperthermia. *J. Therm. Biol.* **63** 124–30
- 8 Travers G J S, Nichols D S, Farooq A, Racinais S and Périard J D 2016 Validation of an ingestible
9 temperature data logging and telemetry system during exercise in the heat. *Temp. (Austin,
10 Tex.)* **3** 208–19
- 11 Wilkinson D M, Carter J M, Richmond V L, Blacker S D and Rayson M P 2008 The Effect of Cool Water
12 Ingestion on Gastrointestinal Pill Temperature *Med. Sci. Sport. Exerc.* **40** 523–8
- 13
- 14